

ORIGINAL RESEARCH

Apical Debris Extrusion during Root Canal Preparation with ProTaper Next and Mani Silk Rotary Systems: An *in vitro* Study

¹Madhusudhana Koppolu, ²Ram Basam, ³Chinni Suneelkumar, ⁴Anumula Lavanya

ABSTRACT

Aim: To evaluate the amount of apically extruded debris after the preparation of root canals in extracted human single-rooted teeth using ProTaper Next and Mani Silk rotary systems.

Materials and methods: A total of 40 freshly extracted human single-rooted teeth with mature apices and straight root canal were selected and similar length were instrumented with ProTaper Next and Mani Silk rotary systems. Debris and irrigant extruded during instrumentation were collected into preweighed Eppendorf tubes. The Eppendorf tubes were then stored in an incubator at 68°C for 5 days. The weight of the extruded debris was determined by subtracting the initial weight from the final weight.

Statistical analysis: Data analysis was carried out using the Statistical Package for the Social Sciences (SPSS) version 20. Postweights were compared with an independent t test for 2 groups.

Results: Both instruments were associated with apical debris extrusion. There was no significant difference between the ProTaper Next and Mani Silk instruments in terms of mean weight of apically extruded debris.

Conclusion: There was no significant difference among the groups in terms of mean weight of apically extruded debris.

Keywords: Apical debris extrusion, Eppendorf tube, Manisilk, Protaper Next.

How to cite this article: Koppolu M, Basam R, Suneelkumar C, Lavanya A. Apical Debris Extrusion during Root Canal Preparation with ProTaper Next and Mani Silk Rotary Systems: An *in vitro* Study. *J Oper Dent Endod* 2016;1(2):66-69.

Source of support: Nil

Conflict of interest: None

INTRODUCTION

Root canal treatment is a procedure in which pulp tissue, bacteria are removed from the root canal system. During chemomechanical preparation, dentin chips, irrigants,

necrotic pulp tissue, and microorganisms from the root canal gain access to periapical tissues, which leads to inflammation and postoperative pain known as “flare up”¹ that disturbs healing of periradicular tissues. Several studies have shown that all instrumentation techniques and instruments cause apical extrusion of debris.²⁻⁴

A common finding of all the studies regarding the apical extrusion of debris and the irrigant was that the instrumentation techniques using a rotational motion tend to produce a less apical extrusion of debris than instrumentation techniques using a push-pull motion.

The amount of apically extruded debris during canal preparation using ProTaper Next and Mani Silk instruments has not been reported.

Therefore, the aim of this *in vitro* study was to assess the amount of apically extruded debris after the root canal preparation using ProTaper Next and Mani Silk instruments.

The null hypothesis was that there would be no difference among the instrumentation systems in terms of amount of apically extruded debris.

MATERIALS AND METHODS

A total of 40 extracted human single-rooted teeth were used. Inclusion criteria for tooth selection were as follows. A single root canal, no visible root caries, no fractures or cracks, no signs of internal or external resorption or calcification, a completely formed apex, and a curvature <5°, in according with protocol established by Schneider. The teeth were radiographed buccolingually and mesio-distally to rule out any atypical canal morphology and to confirm a single canal with single apical foramen. Soft tissue remnants, debris, and dental calculi that are present on the root surface are removed by ultrasonic scaler and the tooth was stored in distilled water. Endodontic access cavities were prepared using diamond burs (Diatech, coltene whaledent, Alstatten, Switzerland) with a high-speed handpiece under water cooling. After preparation of the access cavity, canal patency was established with a size 10-k file (Dentsply Maillefer). Canals with dimensions that exceeded size 15 were discarded and 40 teeth were finally selected that met the dimension criteria. To ensure standardization and to obtain a reference point,

¹Professor and Head, ²Postgraduate Student, ³Professor, ⁴Reader

¹⁻⁴Department of Conservative Dentistry and Endodontics Narayana Dental College, Nellore, Andhra Pradesh, India

Corresponding Author: Madhusudhana Koppolu, Professor and Head, Department of Conservative Dentistry and Endodontics, Narayana Dental College, Nellore, Andhra Pradesh, India, e-mail: drmadhuk15@gmail.com

incisal edges of teeth were flattened using a high-speed bur and the length of all teeth were standardized to 21 mm. A size 10-k file was placed in the canal until it was just visible at the apical foramen, and the working length was established by reducing 1 mm from this point.

Instrumentation and Debris Collection

Experimental model described by Myers and Montgomery⁵ was used (Fig. 1). A hole was created in the cap of an Eppendorf tube and a tooth was inserted to its cemento-enamel junction. A 27-G needle was placed alongside the cap as a drainage cannula and to equalize air pressure inside and outside the Eppendorf tube. Stoppers were then attached to their Eppendorf tubes, and the tubes were fitted into the vials. Eppendorf tubes were weighed to 10⁻⁵ precision using an electrical balance. Three consecutive measurements were taken for each tube, and the mean values were recorded. Forty teeth were numbered and then randomly assigned into 2 groups of 20 specimens each. Each teeth was isolated with rubber dam.

ProTaper Next Group

In this group, initially Sx were used to half of its working length, then X1 (size 17/0.04 taper), X2 (size 25/0.06 taper) were used to full working length with an endodontic motor (x-smart, Dentsply, Maillefer) at a rotational speed of 300 rpm and 2 Ncm torque, according to the manufacturer’s instructions. A gentle in and out brushing motion was used. In each sample, 3 mL of NaOCl and 3 mL of saline were used as irrigation solution between the uses of files.

Mani Silk Group

In this group, root canals were prepared using Mani Silk file system-simple pack with a gentle in and out motion at 500 rpm and 3 Ncm torque with a torque controlled

endodontic motor (x-smart, Dentsply, Maillefer); first, by using 0.08/25 orifice opener and preparing a glide path, and 0.06/25 and 0.06/30 files were of full working length. In each sample, 3 mL of NaOCl and 3 mL of saline were used as irrigation solution between the uses of files.

Evaluation of apically Extruded Debris

Evaluation was completed by a second examiner blinded to group assignment. On completion of the canal preparation, the Eppendorf tubes were removed from the vials. The debris adherent to the external surface of the root apex was collected by washing the root with 1 mL distilled water in the tube. The tubes were stored in an incubator at 68°C for 5 days to evaporate the irrigant solutions before weighing the debris. The net weight of the dry debris was determined by subtracting the original weight of the Eppendorf tube from the gross weight (Table 1).

Statistical Analysis


Data analysis was carried out using the Statistical Package for the Social Sciences (SPSS) version 20. Shapiro-Wilks normality test results showed that weights in both the groups follow the normal distribution. Therefore, parametric methods were applied for the analysis of the data. Basic descriptions were presented in the form of mean and standard deviation. Postweights were compared with an independent t test for two groups (Graph 1). The level of significance was set at p < 0.05 for all tests.

Table 1: Weight of Eppendorf tubes – preweight and postweight in (gm-grams)

Sl. no.	ProTaper next preweight of eppendorf tubes (gm)	ProTaper next postweight of eppendorf tubes (gm)	Mani Silk preweight of eppendorf tubes (gm)	Mani Silk postweight of eppendorf tubes (gm)
1	0.48	0.51	0.56	0.61
2	0.58	0.59	0.55	0.56
3	0.59	0.60	0.56	0.61
4	0.54	0.57	0.55	0.61
5	0.56	0.57	0.56	0.58
6	0.57	0.59	0.55	0.56
7	0.56	0.58	0.55	0.58
8	0.56	0.61	0.58	0.59
9	0.56	0.58	0.58	0.60
10	0.55	0.60	0.55	0.56
11	0.54	0.59	0.57	0.63
12	0.57	0.62	0.54	0.55
13	0.58	0.62	0.57	0.59
14	0.57	0.58	0.58	0.62
15	0.57	0.62	0.56	0.57
16	0.56	0.57	0.56	0.57
17	0.55	0.57	0.55	0.57
18	0.55	0.62	0.54	0.55
19	0.54	0.56	0.58	0.59
20	0.55	0.56	0.55	0.56



Fig. 1: Experimental model system used to evaluate debris extrusion

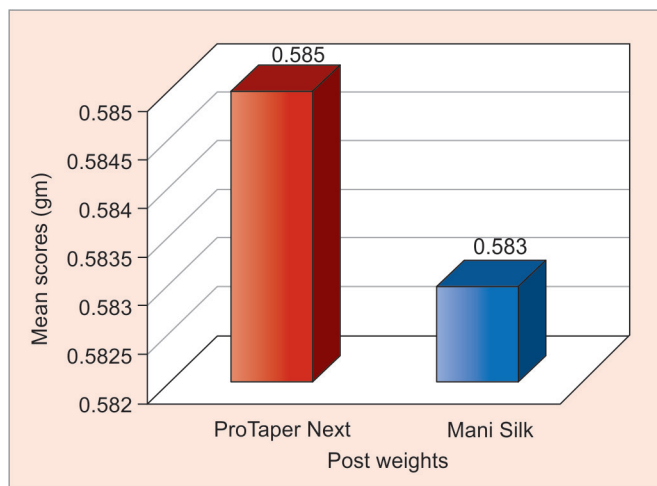

Graph 1: Independent t test was performed between two groups

RESULTS

The mean values and standard deviations for both groups are listed in Table 2. The apical debris extrusion was seen in all specimens. There was no significant difference among the groups in terms of mean weight of apically extruded debris ($p > 0.05$). Thus, the null hypothesis of the present study was accepted.

DISCUSSION

Most influential factor for neuropeptide expression (Substance-P and CGRP) after root canal preparation is the design of the instrument, regardless of the number of files or the type of movement.⁶ Postoperative pain following root canal treatment is related with extrusion of debris during root canal preparation.⁷ Therefore, a reduction in debris extrusion during canal preparation will reduce postoperative pain during or after root canal treatment.⁸

In this study, two different NiTi rotary systems were evaluated in terms of apical debris extrusion using a commonly accepted methodology.⁹ This methodology could be disadvantageous, since there is no apical barrier to mimic the periodontal ligament against the apical extrusion.

The main parameter of the file that causes apical extrusion of debris is cross-section of file and design of file. ProTaper Next¹⁰ (Dentsply Maillefer, Ballaigues, Switzerland) is a fifth-generation NiTi system. These

files incorporate a new M-Wire alloy. The design features include off set-rectangular cross-section¹¹ design for greater strength and less debris extrusion, unique asymmetric rotary motion that further enhances shaping efficiency, and variable tapers. ProTaper Next files are manufactured using M-Wire NiTi to enhance both flexibility and cyclic fatigue resistance. Various studies reported that M-Wire provides superior flexibility and resistance to cyclic fatigue than conventional NiTi alloy, and retains its cutting efficiency.^{12,13}

Mani Silk file¹⁴ has unique cross-sectional tear drop design that cuts exceptionally well and resists fractures, which eliminates the “screwing-in” effect common with many other systems, while removing debris effectively and reducing instrument stress. Ground-breaking proprietary heat treatment provides excellent flexibility without scarifying efficiency and safety. Mani Silk files are available in simple pack – for straight canals, standard pack – for mildly curved canals, complex pack – for moderately and severely curved canals. In this study, Mani Silk-simple pack files were used for straight canals.

The results of the present study revealed that both instrument systems cause apical extrusion of debris during canal preparation. This is consistent with other apical extrusion studies,¹⁵⁻¹⁷ and reinforced the fact that it is impossible to prepare a root canal system chemico-mechanically without apical extrusion of debris. But mechanized instrumentation minimizes the extrusion of debris when compared to manual instrumentation.¹⁸ Both ProTaper Next and Mani Silk rotary systems cause extrusion of debris. Therefore, the null hypothesis of the present study was accepted.

CONCLUSION

The apical debris extrusion was seen in all specimens. There was no significant difference between ProTaper Next and Mani Silk rotary systems in terms of mean weight of apically extruded debris.

REFERENCES

- Seltzer S, Naidorf IJ. Flare-ups in endodontics: I. Etiological factors 1985. J Endod 2004 Jul;30(7):476-481.
- Al-omari MA, Dummer PM. Canal blockage and debris extrusion with eight preparation techniques. J Endod 1995 Mar;21(3):154-158.
- Ustin Y, Canakci BC, Dincer AN, Er O, Duzgun S. Evaluation of apically extruded debris associated with several NiTi systems. Int Endod J 2015 Jul;48(7):701-704.
- Madhusudhana K, Mathew VB, Reddy NM. Apical extrusion of debris and irrigants using hand and three rotary instrumentation systems – an *in vitro* study. Contemp Clin Dent 2010 Oct;1(4):234-236.
- Myers GL, Montgomery S. A comparison of weights of debris extruded apically by conventional filling and Canal Master techniques. J Endod 1991 Jun;17(6):275-279.

Table 2: Mean values and standard deviations for both groups

Groups	Frequency	Mean ± SD	Mean difference	t-value	p-value
Post weights					
ProTaper Next	20	0.585 ± 0.027	0.0025	0.309	0.759
Mani Silk	20	0.583 ± 0.024			

Independent t test was performed between the groups; * $p < 0.05$ (significant), $p > 0.05$ (not significant)

6. Caviedes-Bucheli J, Castellanos F, Vasquez N, Ulate E, Munoz HR. The influence of two rotary-file systems on the apical extrusion of debris and its biological relationship with symptomatic apical periodontitis. A systematic review and meta analysis. *Int Endod J* 2016 Mar;49(3):255-270.
7. Ruiz-Hubard EE, Gutmann JL, Wagner MJ. A quantitative assessment of canal debris forced periapically during root canal instrumentation using two different techniques. *J Endod* 1987 Dec;13(12):554-558.
8. Kocak MM, Cicek E, Kocak S, Salgam BC, Ylmaz N. Apical extrusion of debris using ProTaper Universal and ProTaper Next rotary systems. *Int Endod J* 2015 Mar;48(3):283-286.
9. Karatas E, Arslan H, Kirici DO, Alsancak M, Capar ID. Quantitative evaluation of apically extruded debris with twisted file adaptive instruments in straight root canals: Reciprocation with different angles, adaptive motion, and continuous rotation. *Int Endod J* 2016 Apr;49(4):382-385.
10. ProTaper Next: directions for use. Available from: <http://www.protapernext.com/benefits-concept.html>.
11. Elnaghy AM. Cyclic fatigue resistance of ProTaper Next nickel-titanium rotary files. *Int Endod J* 2014 Nov;47(11):1034-1039.
12. Alapati SB, Brantley WA, Iijima M, Clark WA, Kovarik L, Buie C, Liu J, Ben Johnson W. Metallurgical characterization of a new nickel-titanium wire for rotary endodontic instruments. *J Endod* 2009 Nov;35(11):1589-1593.
13. Zhou H, Peng B, Zheng YF. An overview of the mechanical properties of nickel-titanium endodontic instruments. *Endod Top* 2013 Sep;29(1):42-54.
14. Mani Silk files: directions for use. Available from: <http://www.mani.co.jp>.
15. Burklein S, Benten S, Schafer E. Quantitative evaluation of apically extruded debris with different single-file systems: Reciproc, F360 and OneShape versus Mtwo. *Int Endod J* 2014 May;47(5):405-409.
16. De-Dues G, Neeves A, Silva EJ, Mendonça TA, Lourenço C, Calixto C, Lima EJ. Apically extruded dentin debris by reciprocating single-file and multi-file rotary system. *Clin Oral Investig* 2015 Mar;19(2):357-361.
17. Kirchhoff AL, Fariniuk LF, Mello I. Apical extrusion of debris in flat-oval root canals after using different instrumentation systems. *J Endod* 2015 Feb;41(2):237-241.
18. De-Deus GA, Nogueira Silva EJ, Moreria EJ, de Almeida Neves A, Belladonna FG, Tameirao M. Assessment of apically extruded debris produced by the self-adjusting file system. *J Endod* 2014 Apr;40(4):526-529.